
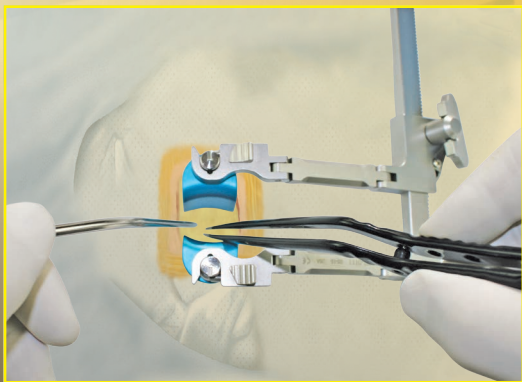


# **NSI**

# **CLEAR-LINE TC**

## **Tethered Cord Pediatric Spinal Retractor**

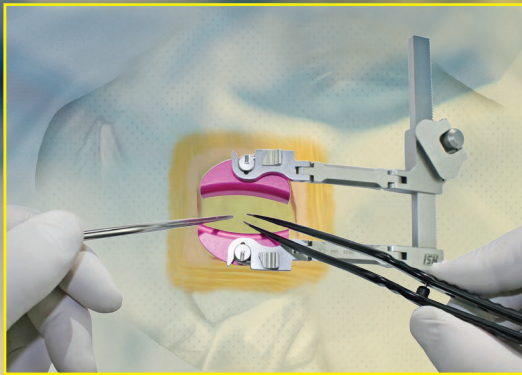

- **IDEAL EXPOSURE**
- **PEDIATRIC APPLICATION**  
**BLADE DEPTHS**

303-860-0261  
[www.nsi-healthsystems.com](http://www.nsi-healthsystems.com)

# IDEAL EXPOSURE


# NSI CLEAR-LINE TC

Application Specific Blade Depths  
(15mm, 20mm, 25mm, 30mm, 35mm)



46 mm wide blades

Low Profile / Minimal Exposure

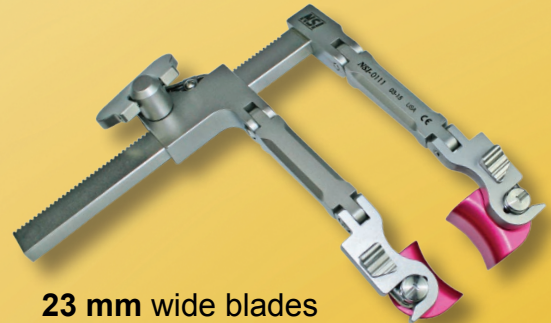

23 mm wide blades



## NSI-9001 Clear-Line Tethered Cord / Pediatric Spinal Retractor

NSI-0111	SLS Transverse Retractor (Standard)	1	NSI-4615SS	46x15mm SLS-ST Multi-Level Blade	2
NSI-0098	SLS Screw-On Retractor Handle	2	NSI-4620SS	46x20mm SLS-ST Multi-Level Blade	2
NSI-2315SS	23x15mm SLS Short Teeth Blade	2	NSI-4625SS	46x25mm SLS-ST Multi-Level Blade	2
NSI-2320SS	23x20mm SLS Short Teeth Blade	2	NSI-4630SS	46x30mm SLS-ST Multi-Level Blade	2
NSI-2325SS	23x25mm SLS Short Teeth Blade	2	NSI-4635SS	46x35mm SLS-ST Multi-Level Blade	2
NSI-2330SS	23x30mm SLS Short Teeth Blade	2	575-801	TC Retractor Sterilization Case	1
NSI-2335SS	23x35mm SLS Short Teeth Blade	2			